

# SHENITECH AG

Purchase Order Number: 000120  
ULTRASONIC METER ON 3" CS SCH 40 PIPE #3-60  
Unit Serial Number: 06080244H  
M1 Transducer Type  
Calibration Factor = 0.9280

CALIBRATION  
DATE: October 25, 2006


Run #	Line Temp Deg F	Net Weight lb.	Run Duration secs.	Flow GPM	Total Gallons ARL	Reading Device Gallons	Dev. Tot. Gal divided by Tot. Gal. ARL
10	48	2537.4	360.424	50.68	304.48	304.95	1.0015
11	48	9560.1	333.807	206.1	1147.17	1150.76	1.0031
12	48	5561.5	373.886	107.0	667.36	660.95	0.9904
13	48	7562.2	347.458	156.6	907.43	901.23	0.9932
14	48	9570.7	275.133	250.4	1148.44	1146.23	0.9981
15	48	9584.7	230.600	299.2	1150.13	1147.87	0.9980
16	48	9579.4	172.529	399.7	1149.50	1154.36	1.0042

CALIBRATED BY: THL

The data reported on herein was obtained by measuring equipment the calibration of which is traceable to NIST, following the installation and test procedures referenced in this report, resulting in a flow measurement uncertainty of +/- 0.25% or less.

CERTIFIED BY: 



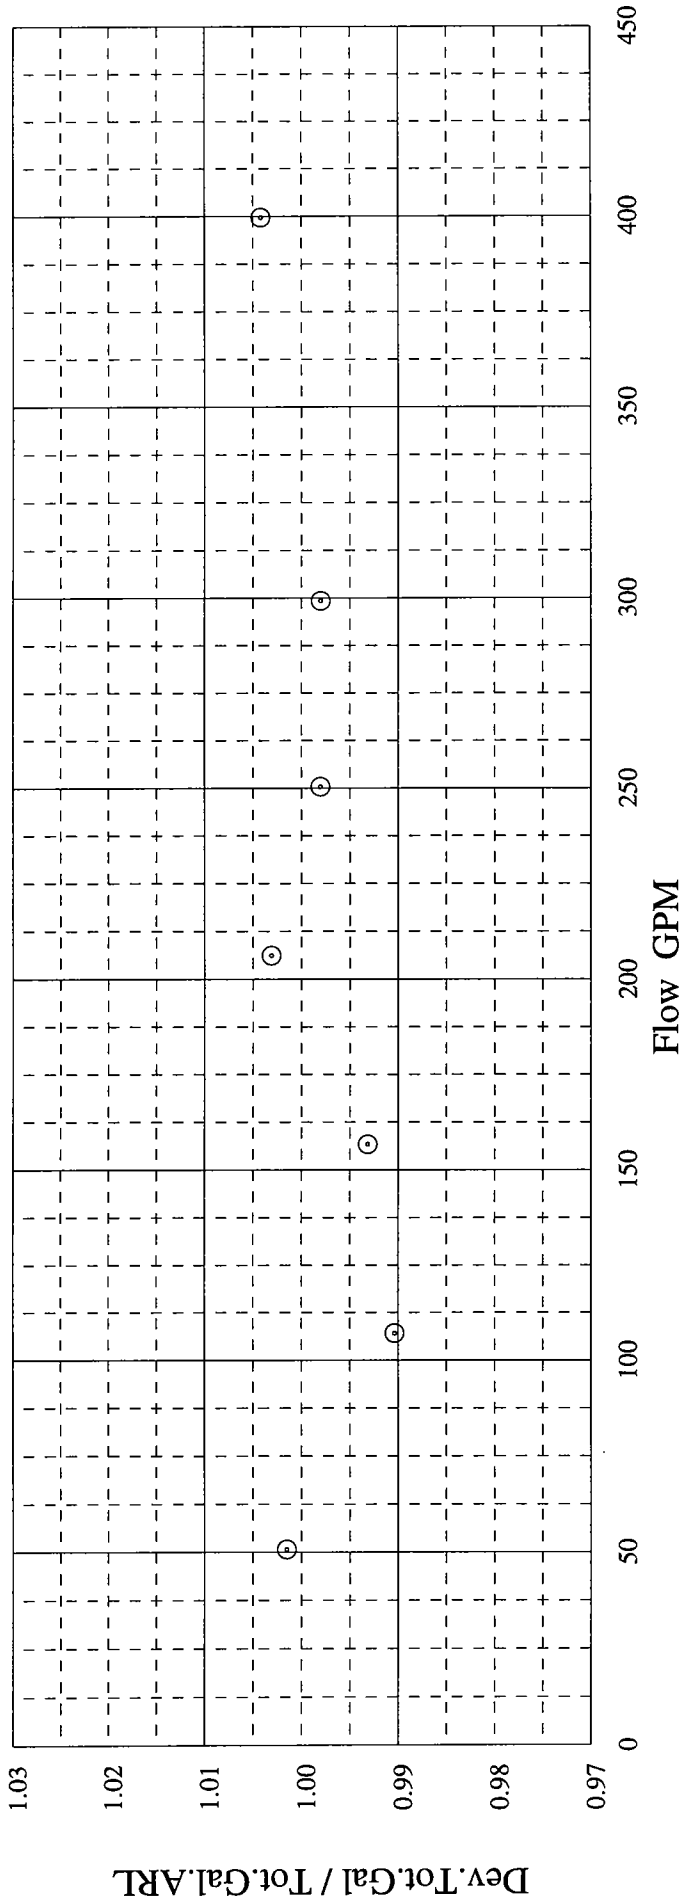

**SHENITECH AG**  
 Purchase Order Number: 000120  
**ULTRASONIC METER ON 3" CS SCH 40 PIPE #3-60**  
 Serial Number: 06080244H  
 M1 Transducer Type  
 October 25, 2006  
 Calibration Factor = 0.9280

Certified By: *James B. Apple*

